



# MACT™ 5 A4/MACT™ 5 A5/MACT™ 5 Lite Resting ECG Analysis System

## MAC 5 A4


1

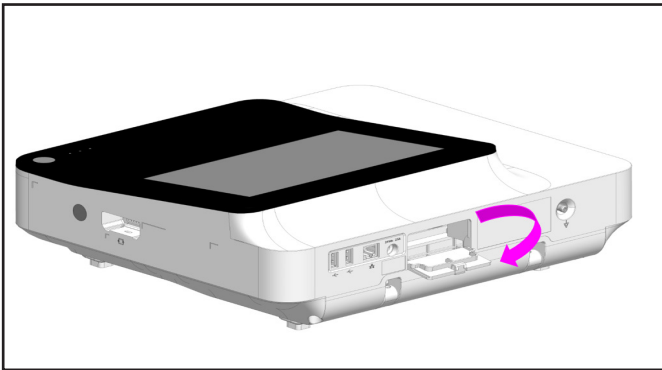


2

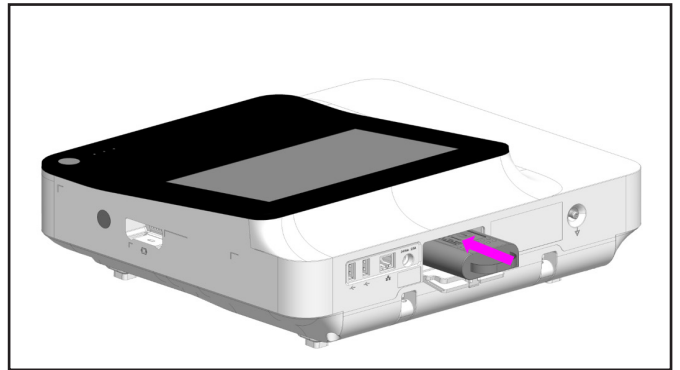


3

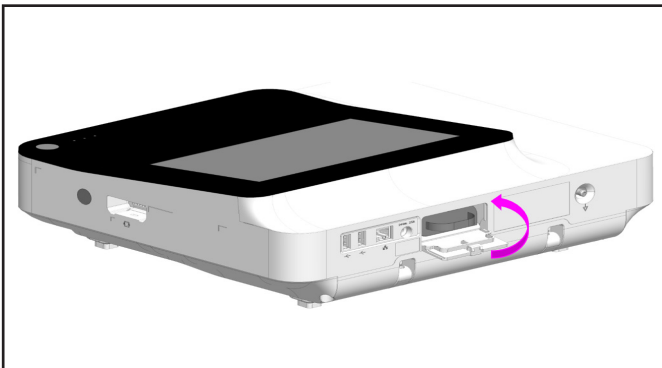


4

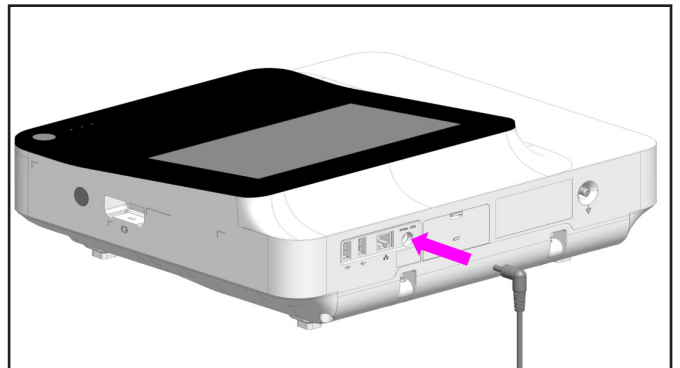

5

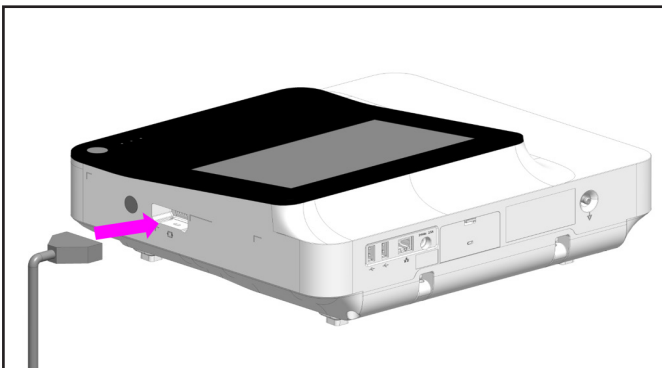


6

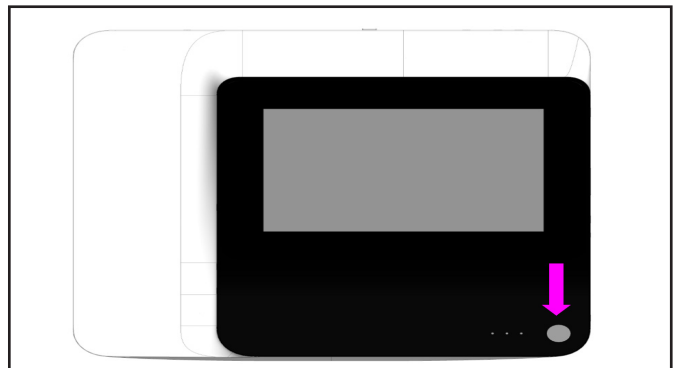


## MAC 5 A5


1

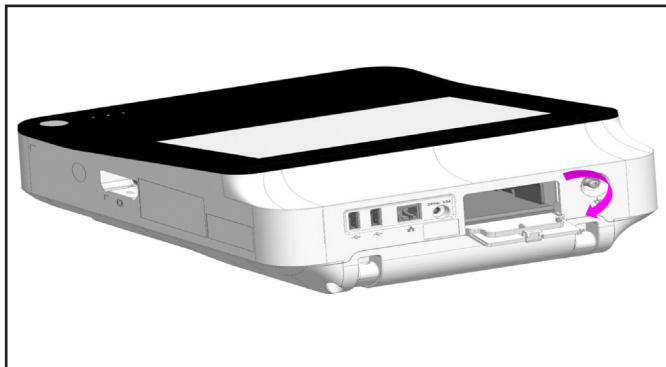


2

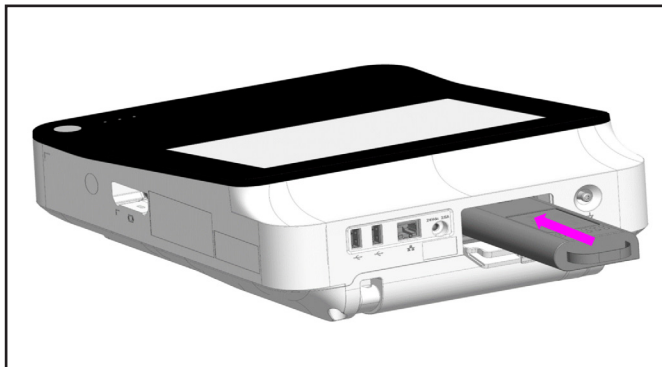


3

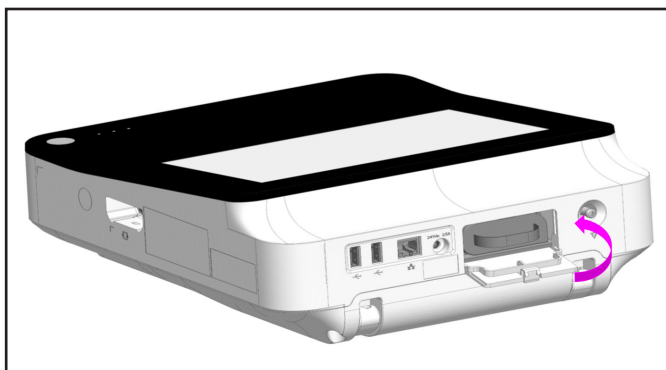


4

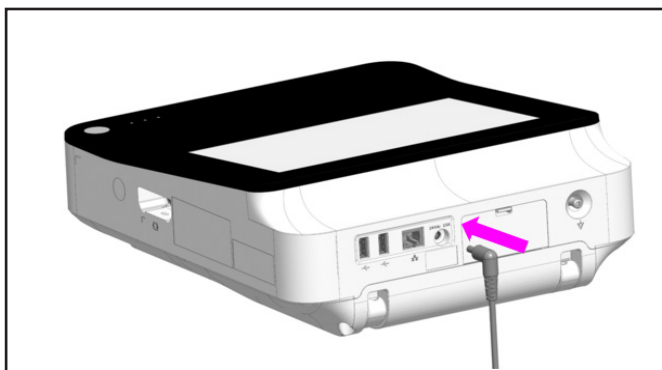

5

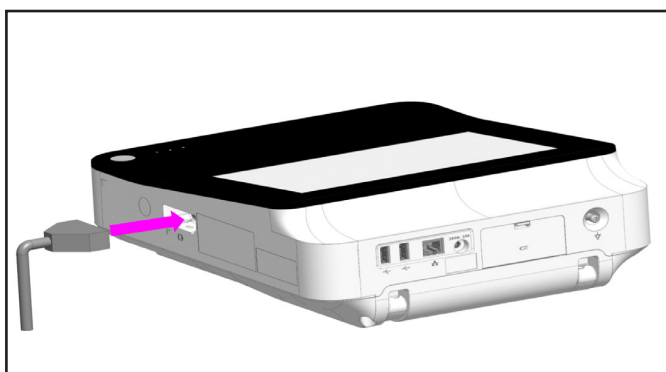


6

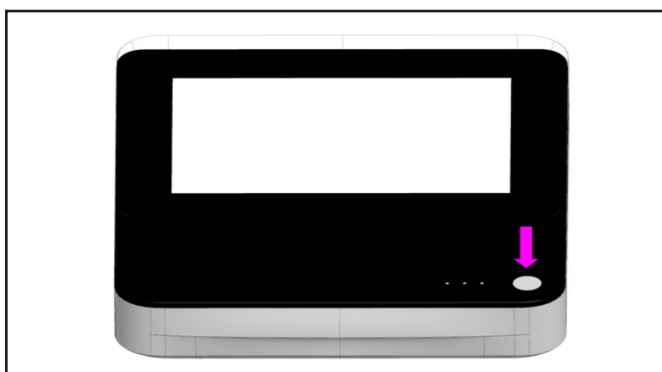


## MAC 5 Lite


1

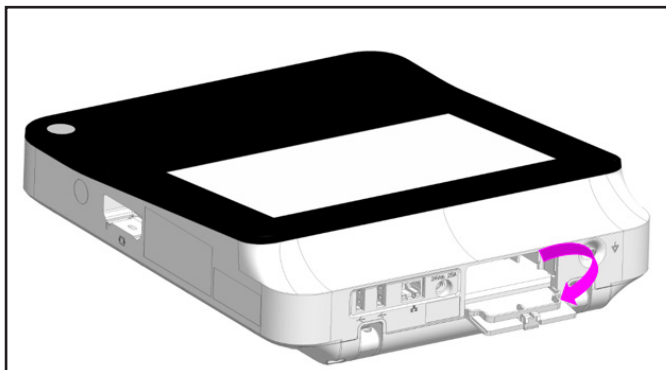


2

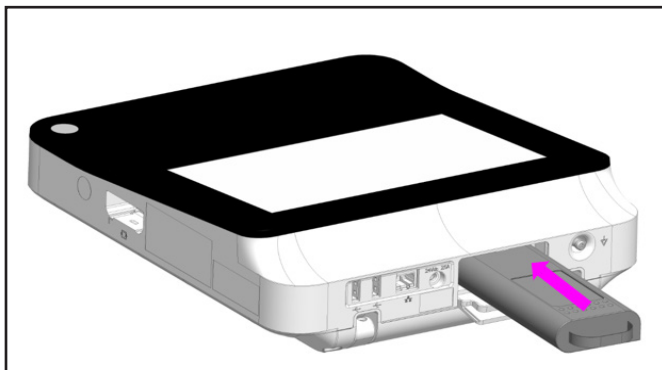


3

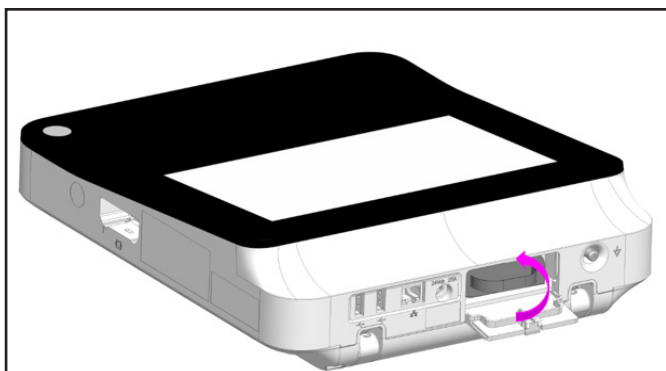


4

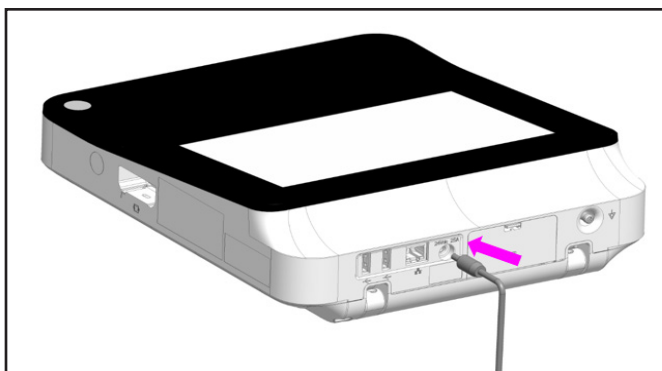

5

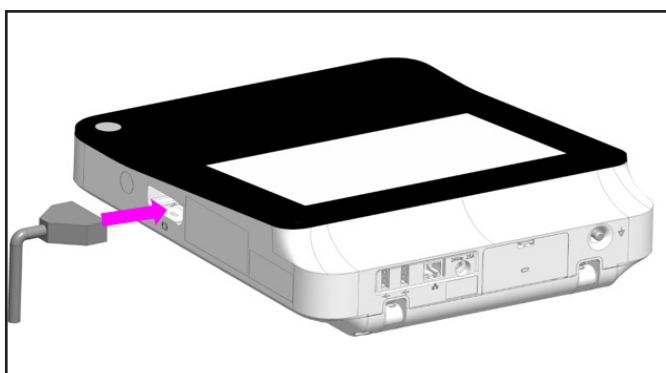


6

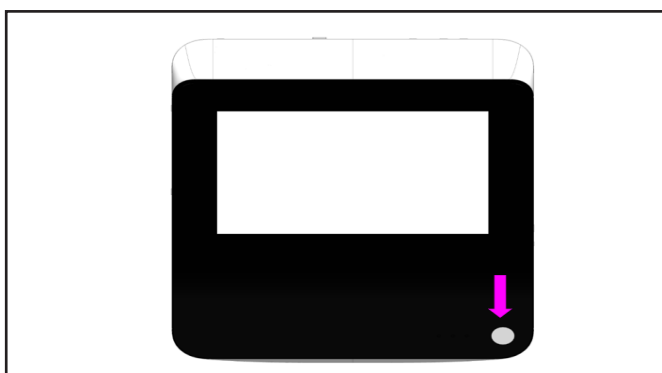


MAC 5 A4/MAC 5 A5

1

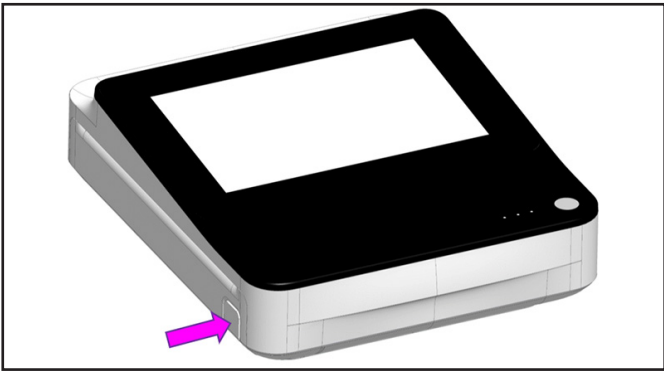


2

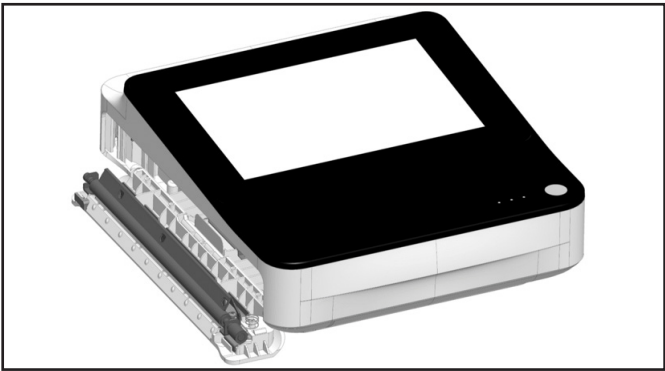


3


Pull the paper pull tab and place the paper above it, but do not remove the paper pull tab from the device.

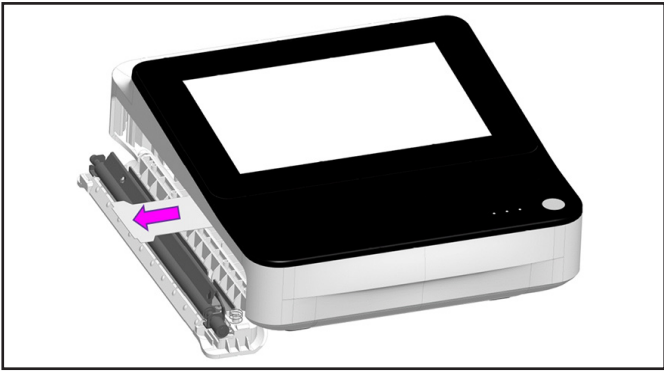


4

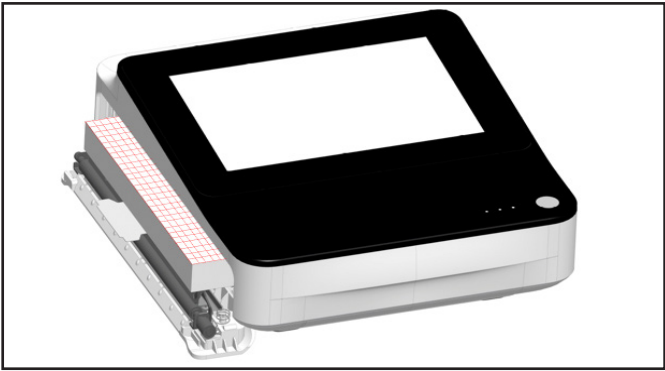

5

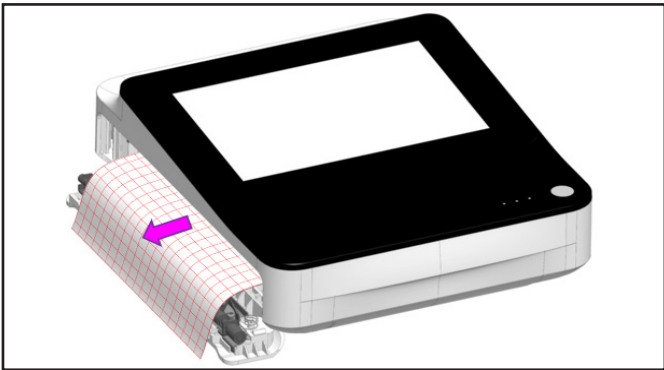

6

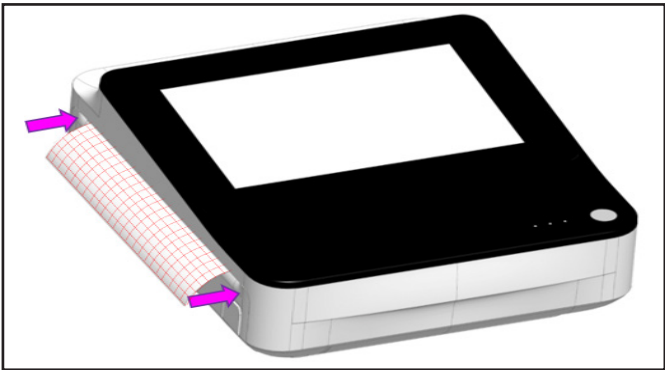

GE Medical Systems  
Information Technologies, Inc.  
9900 Innovation Drive  
Wauwatosa, WI 53226 USA



GE Medical Systems S.C.S.  
283 rue de la Minière  
78530 BUC, France

© 2021-2023 GE HealthCare – All rights reserved. GE is a trademark of General Electric Company used under trademark license.  
GE HealthCare reserves the right to make changes in specifications and features shown herein, or discontinue the product described at any time without notice or obligation.  
The materials contained in this document are intended for educational purposes only. This document does not establish specifications, operating procedures, or maintenance methods for any of the products referenced. Always refer to the official written materials (labeling) provided with the product for specifications, operating procedures, and maintenance requirements. Specifications are subject to change.