

222TD
Facial Chair

SILVERFOX
beauty




Silverfox Corporation Limited

CE FDA RoHS



UNPARALLELED USER EXPERIENCE

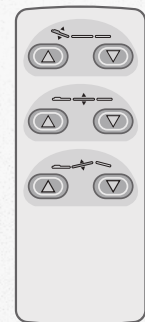

2221D Series Hand Remote ----- Standard Configuration



Trendelenburg

Trendelenburg position(-15 degree), used to treat hypotension or shock during surgery to increase blood perfusion to vital organs. With this function, the electrical beds can be extended to multiple scenarios.

Product Extensions / Family Series



2221D



2220D



2219B

※ Standard Configuration



Hand
Controller



Max Load
Bearing

※ Options



Latex/
Memory Foam





Foot
Controller

※ Technical Parameters

Model	Product	Voltage	Frequency	Power Rating	Warranty
2221D	Facial Chair	AC 100-120V	50/60Hz	300W	2 years (Motors and Control Box: 3 years)

※ General Specifications

- Max load bearing : 200 kg / 440 lbs
- Net weight : 64 kg / 141 lbs
- Gross weight : 77 kg / 170 lbs
- Product size(L*W*H) : 1830x790x620 / 850 (mm) 72x31.1x24.4 / 33.4 (in)
- Package size : 1280x690x690 (mm)≈0.61m³ 50.4x27.2x27.2 (in)≈0.61m³
- Unit:mm / in

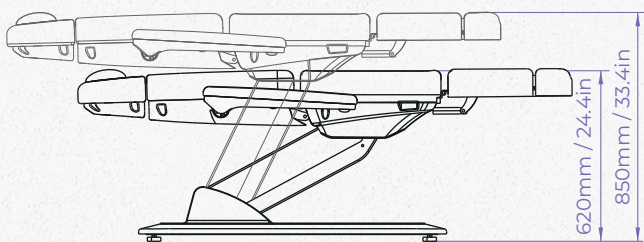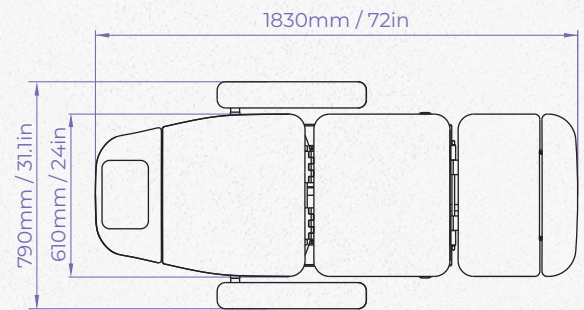

LEATHER COLOR SWATCH

STANDARD LEATHER

LA-A26 White	LA-A178 Light Beige	LA-A69 Coffee Brown
LA-A33 Sand	LA-A68 Gravel	LA-A66 Dark Grey
LA-A06 Shiny Black	LA-A12 Mat Black	LA-A08 Navy Blue
LA-A63 Blue	LA-A351 Lime	

MICROGROOVE LEATHER

LB-A26 White	LB-A01 Light Grey	LB-A69 Coffee Brown
LB-A207 Wine Red	LB-A207 Wine Red	

MICROFIBER LEATHER (OPTION)

LC-A26 White	LC-A33 Sand	LC-A47 Camel Orange
LC-A62 Light Grey	LC-A66 Dark Grey	LC-A12 Mat Black
LC-A932 Purple		


NEW LEATHER (OPTION)

LD-A26 White	LD-A01 Light Grey	LD-A22 Dark Blue
-----------------	----------------------	---------------------

Maintenance

After every treatment, please only use neutral solution to clear the dust, stains on leather, metal part or other parts. Disinfecting solution like alcohol, acid or alkaline solution are forbidden. This is to prevent the lifetime of the components from being shortened.

SPONGE DISSECTION DIAGRAM

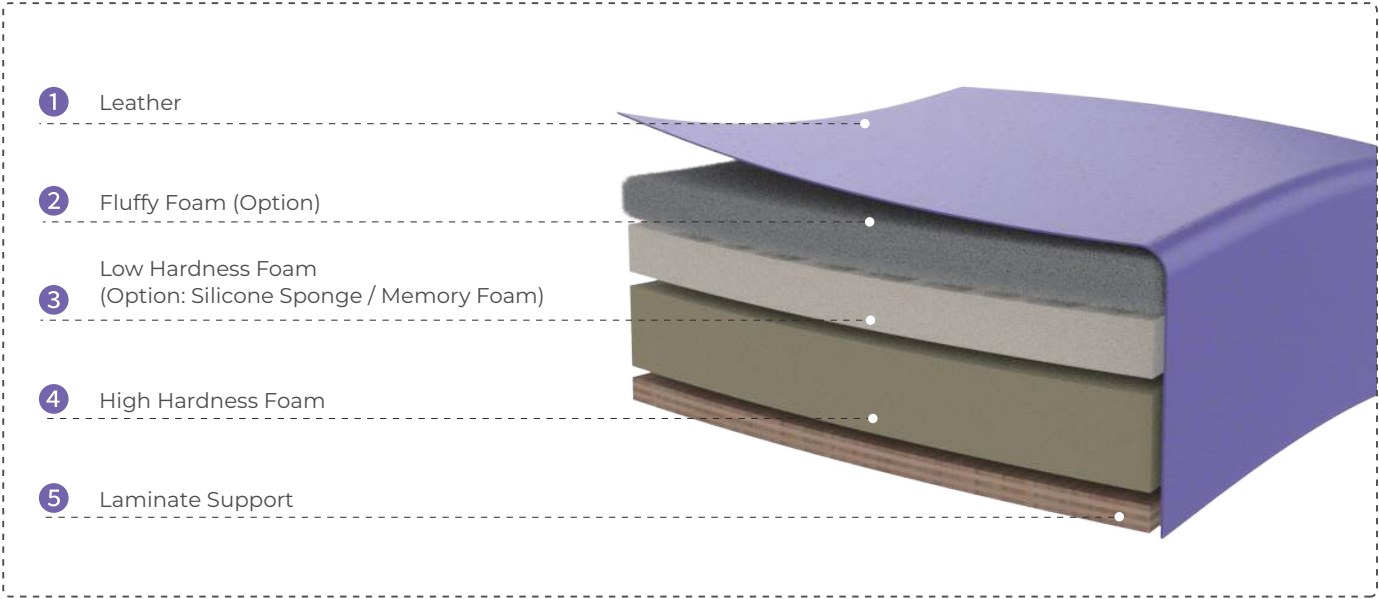

Due to the screen display effect will have color difference, the image is for reference only, the actual color shall prevail.